



DISPOSITIVO DI PRELIEVO STERILE DELLA MISCELA O₂O₃ OXYGEN-OZONE STERILE WITHDRAWAL DEVICE

Check Valve

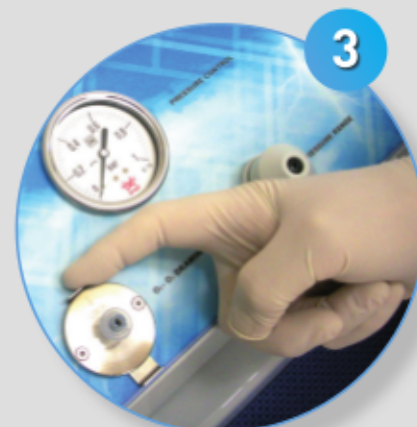

Sistema brevettato di prelievo della miscela di ossigeno-ozono con dispositivo monouso sterile in blister. Garanzia di massima sterilità e sicurezza nel prelievo della miscela gassosa, attraverso l'inserimento della check valve senza contatto con le mani. Valvola creata per oviare possibili infezioni e contestazioni medico-legali che ne possono derivare. Adatta a tutti i tipi di siringa. Possibilità di scaricare all'interno del generatore l'eventuale miscela residua della siringa.

System for withdrawal of gas [O₂O₃] with sterile disposable valves in blister. Maximum sterility conditions guaranteed in the taking of the gaseous mixture, by inserting the component with no hands contact. Valve created in order to obviate possible infections and consequent medical-legal confrontation. Adaptable to all kind of syringes. Possibility to unload, inside the generator, the possible residual mixture in the syringe.

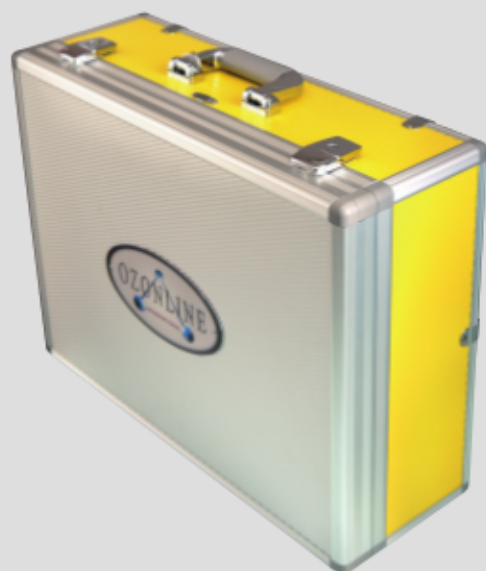

+medica srl

Via Sante Vincenzi, 48 - 40138 Bologna, Italy - Tel. +39 051 308508 - Fax +39 051 6369210
info@medica-srl.com - www.medica-srl.com